



(For scientific research use only, not for clinical diagnosis!)

Rabbit 17-Hydroxycorticosteroid (17-OHCS)

ELISA Kit Instructions for Use Specifications:

48T/96T

**Please read the instructions carefully before use. If you have any questions,
please contact us through the following methods: Official hotline: 025-5229-
8998 Sales department phone: 13914481711 Technical phone: 15950492658
Contact email: 3224949330@qq.com Company website:
www.byabscience.cn For specific shelf life, please see the reagents Box
packaging label. Please use the kit within the shelf life.**

When contacting us, please provide the product number and production date (see box label) so that we can serve you more efficiently.

Nanjing BYabscience technology Co.,Ltd

Website: www.byabscience.cn

Official hotline: 025-5229-8998

Supervision phone number:



Kit performance Detection range: 5

μmol/L-80 μmol/L.

Sensitivity: The lowest detectable dose is less than 0.1 μmol/L.

Precision: intra-batch variation coefficient CV% is less than 10%; inter-batch variation coefficient CV% is less than 15%.

Recovery rate: The recovery rate is between 85%-115%.

Specificity: This kit recognizes native and recombinant rabbit 17-hydroxycorticosteroid (17-OHCS) without crossover to structural analogs. Stability: Stored at 2°C-8°C, validity period is 6 months.

Purpose: Used to detect the concentration of rabbit 17-hydroxycorticosteroid (17-OHCS) in samples such as serum, plasma, cell culture supernatant and tissue.

Shelf life: Stored at 2°C-8°C, valid for 6 months.

Experimental principle

试剂盒采用酶联免疫分析方法。采用生物素标记 17-OHCS，纯化的抗 17-OHCS 抗体包被微孔板，在竞争抑制反应中，一定量的固相抗体与生物素标记 17-OHCS 及非标记抗原（校准品或标本）进行抑制竞争反应，抗体与生物素标记的 17-OHCS 结合量受非标记抗原量所抑制，非标记抗原量多,抗体与生物素标记的 17-OHCS 结合就少，反之结合就多；反应平衡后，形成固相抗体-生物素化 17-OHCS，再加入酶标记的亲合素，形成固相抗体-生物素化 17-OHCS-酶标-亲合素复合物。经加底物显色后，用酶标仪在 450nm 波长下测定吸光度（OD 值）。随着 17-OHCS 浓度的升高，OD 值逐渐下降呈良好的线性关系。本试剂盒具有灵敏度高、特异性强、重复性好、操作简单、快速等特点，对血清中 17-OHCS 的减少或升高有可靠的检出性能。



试剂盒组分与保存 未开封的试剂盒保存在 2-8 度，不得使用过期试剂盒。

组分	48 孔配置	96 孔配置	开封后储存
预包被酶标板	48T	96T	2-8°C 14 天
标准品	0.3mL*6 管	0.3mL*6 管	2-8°C 14 天
样本稀释液	3 ml	6 ml	2-8°C 180 天
生物素化抗原	3 ml	6 ml	2-8°C 14 天
HRP 标记亲和素	3 ml	6 ml	2-8°C 180 天
显色底物 A	3 ml	6 ml	2-8°C 180 天
显色底物 B	3 ml	6 ml	2-8°C 180 天
终止液	3 ml	6 ml	2-8°C 180 天
20×洗液	15 ml	25 ml	2-8°C 180 天
封板膜	2 张	2 张	
说明书	1 份	1 份	
自封袋	1 个	1 个	

校准品浓度依次为：80、40、20、10、5、0 μmol/L。

注意：1：使用前请检查试剂盒中试剂的标签和数量与表格是否一致。

2：如果试剂盒的组份需要再次使用，请确保上一次使用之后没有被污染。

3：酶标板单次未使用完，要谨记密封放到 2-8°C 保存。

试验所需自备试验器材 (不提供，但可协助购买)

1) 能够检测 450 nm 吸光度的酶标仪 2) 移液器及枪头、加样槽 3)

37°C 恒温箱或水浴锅 4) 准备试剂用的试管、离心管、量筒等 5) 蒸馏

水或去离子水

Nanjing BYabscience technology Co.,Ltd

网址: www.byabscience.cn

官方热线: 025-5229-8998

监督电话: 15950492658



6) 涡旋振荡器、微孔板振荡器 注意事项

- 1) 仅供科研使用，不得用于临床诊断。
- 2) 在试剂盒标示的有效期内使用，过期产品不得使用。
- 3) 跟其他厂家的试剂盒或者组分不能混用，使用试剂盒配套的样品稀释液。
- 4) 如果样本值高于最高标准品浓度值，请将样本适当稀释后，再重新测定。
- 5) 待测样本中存在的人抗鼠等异嗜抗体会干扰检测结果，检测前，请排出该因素。
- 6) 通过其他方法得到的检测结果，与本试剂盒测定结果不具有直接的可比性。
- 7) 试验中请穿着实验服并戴乳胶手套做好防护工作。特别是检测血液或者其他体液样品时，请按国家生物实验室安全防护条例执行。
- 8) 严格按照规定的时间和温度进行温育以保证准确结果。所有试剂都必须在使用前达到室温 20-25°C。使用后立即冷藏保存试剂。
- 9) 洗板不正确会导致不准确的结果。在加入底物前确保尽量吸干孔内液体。温育过程中不要让微孔干燥掉。
- 10) 消除板底残留的液体和手指印，否则影响 OD 值。
- 11) 底物显色液应呈无色或很浅的颜色。
- 12) 避免试剂和标本的交叉污染以免造成错误结果。
- 13) 在储存和温育时避免强光直接照射。
- 14) 检测使用的酶标仪需要安装能检测 450±10nm 波长的滤光片，光密度范围在 0-3.5 之间。建议使用时提前 15 分钟预热。
- 15) 试验中所用的 EP 管和吸头均为一次性使用，严禁混用。



样品的准备和保存

以下只是列出样品采集和保存的一般指南。所有样本采集保存过程中，不得使用叠氮钠做为防腐剂。样品如果不立即分析，应分装后冷冻保存，且避免反复冻融。

细胞培养上清——离心去除沉淀，立即分析或分装后-20℃冷冻保存。

Serum - Collect blood in a clean test tube, coagulate at room temperature for 30 minutes, centrifuge at 2000×g for 20 minutes, and collect serum. Analyze immediately or aliquot and store frozen at -20°C.

Plasma—anticoagulate with heparin, citrate, or EDTA, and centrifuge at 2000×g for 20 minutes at 2-8°C within 30 minutes of blood draw. To eliminate the influence of platelets, it is recommended to further centrifuge at 10,000 × g for 10 minutes at 2-8°C. Analyze immediately or aliquot and store frozen at -20°C.

Cell lysis buffer - For adherent cells, remove the culture medium and wash with PBS, normal saline or serum-free culture medium. Add an appropriate amount of lysis solution and pipet several times with a gun to fully contact the lysate and cells. Typically after 10 seconds, cells are lysed. For suspended cells, collect the cells by centrifugation and wash them with PBS, physiological saline or serum-free culture medium. Add an appropriate amount of lysis solution, blow the cells with a gun, and flick them with your fingers to fully lyse the cells. After full lysis, centrifuge at 10000-14000×g for 3-5 minutes and take the supernatant. Analyze immediately or aliquot and store frozen at -20°C.

Tissue homogenate - rinse the tissue with pre-cooled PBS (0.01M, pH=7.4) to remove residual blood (lysed red blood cells in the homogenate will affect the measurement results), weigh and cut the tissue into pieces. Mix the minced tissue with the corresponding volume of PBS (generally at a weight-to-volume ratio of 1:9, for example, 1g of tissue sample corresponds to 9mL of PBS.

The specific volume can be adjusted appropriately according to experimental needs and

recorded. It is recommended to add Protease inhibitor) was added to a glass homogenizer and ground thoroughly on ice. In order to further lyse tissue cells, the homogenate can be sonicated or repeatedly frozen and thawed. Finally, centrifuge the homogenate at $5000 \times g$ for 5 to 10 minutes, and take the supernatant for detection.

Urine - Collect in sterile tubes and centrifuge at $2000 \times g$ for 20 minutes. Carefully collect the supernatant. If a precipitate forms, centrifuge again.

Nanjing BYabscience technology Co.,Ltd

Website: www.byabscience.cn

Official hotline: 025-5229-8998

Supervision phone number:



Reagent preparation 1. Before use, all components must be rewarmed

for at least 60 minutes to ensure sufficient rewarming to room

temperature.

2. Concentrated washing liquid: The concentrated washing liquid taken out from the refrigerator will produce crystals. This is a normal phenomenon. Heating in a water bath will completely dissolve the crystals. Concentrated detergent and distilled water, dilute 1:20, that is, 1 part of concentrated detergent, add 19 parts of distilled water.

Operating procedures: Return all reagents and components to room temperature first. It is recommended to do duplicate holes for standards, quality control materials and samples.

1. Prepare the working solution of various components of the kit according to the method described in the previous instructions.

2、从铝箔袋中取出所需板条，剩余的板条用自封袋密封放回冰箱。

3、将预包被板从密封袋中取出，设一个空白对照孔，不加任何液体；每个校准品设 2 孔，每孔加入对应校准品 50 μ l；其余每个检测孔直接加待测血清或质控品 50 μ l。

4、除空白孔外所有孔加入生物素化抗原 50 μ l，混匀，贴上封板膜，置 37 $^{\circ}$ C 温育 60 分钟。

5、手工洗板：弃去孔内液体，洗涤液注满各孔，静置 10 秒甩干，重复 3 次后拍干。洗板机洗板：选择洗涤 3 次程序洗板后拍干。

（提示：为获得理想的实验结果，必须彻底移除残留液体。洗板完成之后，请立即进行下一步操作，不要让微孔板干燥。）6、每孔加入酶标亲和素 50 μ l（空白对照孔除外），混匀，贴上封板膜，置 37 $^{\circ}$ C 温育 30 分钟。

7、手工洗板：弃去孔内液体，洗涤液注满各孔，静置 10 秒甩干，重复 3 次后拍干。洗板机洗

板：选择洗涤 3 次程序洗板后拍干。

8、每孔加显色剂 A 50 μ l，显色剂 B 50 μ l，振荡混匀后，置 37 $^{\circ}$ C 避光显色 15 分钟，每孔加终止液 50 μ l。

9、用酶标仪读数，取波长 450nm，先用空白对照孔调零点，然后测定各孔光密度值（OD 值）。

Nanjing BYabscience technology Co.,Ltd

网址：www.byabscience.cn


官方热线：025-5229-8998

监督电话：15950492658



结果计算

9、以标准品浓度做为横坐标，对应的吸光度（OD 值）作为纵坐标，利用计算机软件，采用四参数 Logistic 曲线拟合（4-p1），创建标准曲线方程，通过样品的吸光度（OD 值），利用方程计算样品的浓度值。【用 ELISA Calc 软件计算】10、如果样品被稀释，通过上述方法测的的浓度值，要乘以稀释倍数，才是样品的最终浓度。注意：实验者需根据自己的实验建立标准曲线。每次检测，每块酶标板都必须设立标准曲线。以下曲线仅供参考！

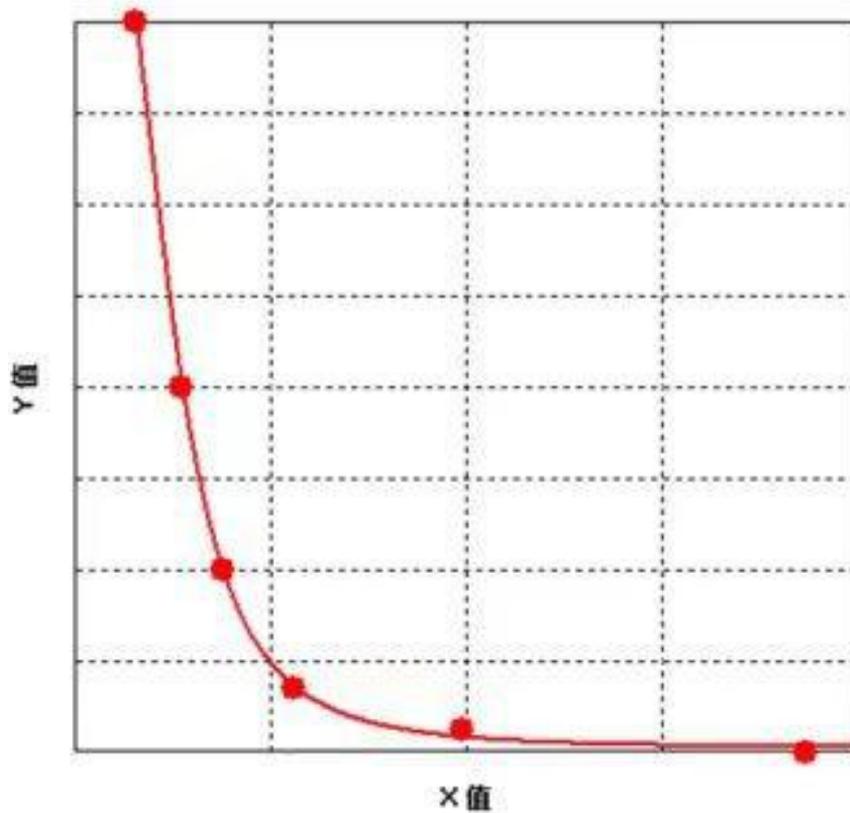

（标曲示意图，仅供参考）

Nanjing BYabscience technology Co.,Ltd



[Problem Analysis] If the experimental results are not good, please take pictures of the color development results in time, save the experimental data, keep the used strips and unused reagents, and then contact our company's technical support to solve the problem for you. At the same time, you can also refer to the following information:

[Questions and Answers]

Problem description	Possible reasons	Corresponding countermeasures Corresponding countermeasures
standard curve gradient difference	Incorrect liquid aspiration or	Check pipettes and tips
	Equilibration time is too short	Ensure sufficient balancing time
	Incomplete washing	Ensure the washing time and number of washings and the amount of liquid added to each hole
Very weak or colorless	Incubation time too short	Ensure adequate incubation time
	The experimental temperature is incorrect	Use recommended experimental temperatures
	Insufficient reagent volume or missing addition	Check the liquid aspirating and adding process to ensure that all reagents are added in order and in
	Incorrect dilution	
	Enzyme label inactivation or substrate failure	Mix enzyme conjugate and substrate and check by rapid color development
Reading value is low	Microplate reader settings are incorrect	Check the wavelength and filter
		Turn on the microplate reader and preheat it in advance
Large coefficient of variation	Adding fluid incorrectly	Check the filling situation
High background value	The working concentration of the	Use the recommended dilution
	Incomplete washing of enzyme plate	Ensure that each step of cleaning is complete; if using an automatic plate washer, please check whether all outlets are blocked;
	The lotion is contaminated	Prepare fresh lotion
Low sensitivity	Improper storage of ELISA kits	Store relevant reagents according to
	Not terminated before reading	Stop solution should be added to

Nanjing BYabscience technology Co.,Ltd

Website: www.byabscience.cn

Official hotline: 025-5229-8998

Supervision phone number: