



**(For scientific research use only, not for clinical diagnosis!)**

## **Rat Mannose Binding Protein-Associated Serine Protease 2**

**(MASP-2) ELISA Kit Instructions for Use Product No.: BY-**

**ER337836 Specifications: 48T/96T Detection Range: 62.5 pg/mL–  
2000 pg/mL.**

**Sensitivity:** The lowest detectable dose is less than 10 pg/mL.

**Precision:** intra-batch variation coefficient CV% is less than 10%; inter-batch variation coefficient CV% is less than 15%.

**Recovery rate:** The recovery rate is between 85%-115%.

**Specificity:** This kit recognizes native and recombinant rat mannose-binding protein-associated serine protease 2 (MASP-2) and has no crossover with structural analogs.

**Stability:** Stored at 2°C–8°C, validity period is 6 months.

**Purpose:** Used to detect the concentration of rat mannose-binding protein-associated serine protease 2 (MASP-2) in samples such as serum, plasma, cell culture supernatant, and tissue.

**Please read the instructions carefully before use. If you have any questions,  
please contact us through the following methods: Official hotline: 025-5229-  
8998 Sales department phone: 13914481711 Technical phone: 15950492658**

**Company website: [www.byabscience.cn](http://www.byabscience.cn) For the specific shelf life, please  
refer to the outer packaging label of the kit. Please use the kit within the  
shelf life.**

**Nanjing BYabscience technology Co.,Ltd**

**Website: [www.byabscience.cn](http://www.byabscience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**



When contacting us, please provide the product number and production date (see box label) so that we can serve you more efficiently.



## Experimental principle

This kit uses a double-antibody sandwich enzyme-linked immunosorbent assay (ELISA). In the microwell microplate pre-coated with anti-rat mannose-binding protein-associated serine protease 2 (MASP-2) antibody (solid-phase antibody), add rat mannose-binding protein-associated serine protease 2 (MASP-2) Calibrator and sample to be tested, then add HRP-labeled anti-rat mannose-binding protein-associated serine protease 2 (MASP-2) antibody (enzyme-labeled antibody), after incubation and sufficient washing, remove unbound components, and A sandwich complex of solid-phase antibody-antigen-enzyme-labeled antibody is formed on the solid surface of the microplate. Adding substrates A and B, the substrates are catalyzed by HRP to produce a blue product, which is finally converted into yellow under the action of the stop solution (acidic solution). The absorbance (OD value) was measured on a microplate reader at a wavelength of 450 nm. The absorbance (OD value) was positively correlated with the concentration of rat mannose-binding protein-associated serine protease 2 (MASP-2) in the sample to be tested. The concentration of rat mannose-binding protein-associated serine protease 2 (MASP-2) in the sample can be calculated by fitting the calibrator curve.

## Experimental schematic diagram



**Nanjing BYabsience technology Co.,Ltd**

**Website:** [www.byabsience.cn](http://www.byabsience.cn)

**Official hotline:** 025-5229-8998

**Supervision phone number:**



**Kit components and storage: Store unopened kits at 2-8 degrees Celsius. Do not use expired kits.**

Components	48-well configuration	96-well configuration	Store after opening
Pre-coated enzyme plate	48T	96T	<b>2-8°C 14 days</b>
Standard product	0.3mL*6 tubes	0.3mL*6 tubes	<b>2-8°C 14 days</b>
sample diluent	3ml	6ml	2-8°C 180 days
HRP labeled antibodies	5ml	10ml	<b>2-8°C 14 days</b>
Chromogenic substrate A	3ml	6ml	2-8°C 180 days
Chromogenic substrate B	3ml	6ml	2-8°C 180 days
stop solution	3ml	6ml	2-8°C 180 days
<b>20×Lotion</b>	15ml	25ml	2-8°C 180 days
sealing film	2 sheets	2 sheets	
manual	1 serving	1 serving	
Ziplock bag	1	1	

The concentrations of calibrators are: 2000, 1000, 500, 250, 125, 62.5 pg/mL.

Note: 1: Before use, please check whether the label and quantity of the reagents in the kit are consistent with the table.

2: If the components of the kit need to be used again, please ensure that they have not been contaminated since the last use. 3: If the enzyme plate is not used up in a single time, remember to seal it and store it at 2-8°C.

**Prepare your own test equipment required for the test (not provided, but can assist in**

1) Microplate reader capable of detecting absorbance at 450 nm 2) Pipette, pipette tip, and sample addition tank 3) 37°C incubator or water bath 4) Test tubes, centrifuge tubes, measuring cylinders, etc. for preparing

reagents 5) Distilled water or deionized

water Ionized water

**Nanjing BYabsience technology Co.,Ltd**

**Website: [www.byabsience.cn](http://www.byabsience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**



6) Vortex shaker, microplate shaker

**Notes 1) For scientific research use only,  
not for clinical diagnosis.**

- 2) Use within the validity period marked on the kit. Expired products must not be used.
- 3) Do not mix with kits or components from other manufacturers. Use the sample diluent provided with the kit.
- 4) If the sample value is higher than the highest standard concentration value, please dilute the sample appropriately and then re-measure.
- 5) Human anti-mouse and other heterophilic antibodies present in the sample to be tested will interfere with the test results. Please eliminate this factor before testing.
- 6) The test results obtained by other methods are not directly comparable to the test results of this kit.
- 7) Please wear a lab coat and latex gloves for protection during the test. Especially when testing blood or other body fluid samples, please follow the national biological laboratory safety protection regulations.
- 8) Carry out incubation strictly according to the specified time and temperature to ensure accurate results. All reagents must reach room temperature 20-25°C before use. Store reagents refrigerated immediately after use.
- 9) Improper plate washing can lead to inaccurate results. Make sure to absorb as much liquid as possible from the wells before adding substrate. Do not allow the microwells to dry out during incubation.
- 10) Eliminate residual liquid and fingerprints on the bottom of the plate, otherwise it will affect the OD value.
- 11) The substrate chromogenic solution should be colorless or very light in color.
- 12) Avoid cross-contamination of reagents and specimens to avoid erroneous results.



- 13) Avoid direct exposure to strong light during storage and incubation.
- 14) The microplate reader used for detection needs to be equipped with a filter capable of detecting a wavelength of  $450\pm 10\text{nm}$ , and the optical density range is between 0-3.5. It is recommended to preheat 15 minutes in advance before use.
- 15) The EP tubes and tips used in the test are single-use and are strictly prohibited from mixing.

**Nanjing BYabscience technology Co.,Ltd**

**Website: [www.byabscience.cn](http://www.byabscience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**



## Sample preparation and storage

The following lists only general guidelines for sample collection and preservation. During the collection and storage of all samples, sodium azide shall not be used as a preservative. If the sample is not analyzed immediately, it should be aliquoted and stored frozen, and repeated freezing and thawing should be avoided.

**Cell culture supernatant - centrifuge to remove precipitate, analyze immediately or aliquot and store frozen at -20°C.**

**Serum - Collect blood in a clean test tube, coagulate at room temperature for 30 minutes, centrifuge at 2000×g for 20 minutes, and collect serum. Analyze immediately or aliquot and store frozen at -20°C.**

**Plasma—anticoagulate with heparin, citrate, or EDTA, and centrifuge at 2000×g for 20 minutes at 2-8°C within 30 minutes of blood draw. To eliminate the influence of platelets, it is recommended to further centrifuge at 10,000 × g for 10 minutes at 2-8°C. Analyze immediately or aliquot and store frozen at -20°C.**

**Cell lysis buffer - For adherent cells, remove the culture medium and wash with PBS, normal saline or serum-free culture medium. Add an appropriate amount of lysis solution and pipet several times with a gun to fully contact the lysate and cells. Typically after 10 seconds, cells are lysed. For suspended cells, collect the cells by centrifugation and wash them with PBS, physiological saline or serum-free culture medium. Add an appropriate amount of lysis solution, blow the cells with a gun, and flick them with your fingers to fully lyse the cells. After full lysis, centrifuge at 10000-14000×g for 3-5 minutes and take the supernatant. Analyze immediately or aliquot and store frozen at -20°C.**

**Tissue homogenate - rinse the tissue with pre-cooled PBS (0.01M, pH=7.4) to remove residual blood (lysed red blood cells in the homogenate will affect the measurement results), weigh and cut the tissue into pieces. Mix the minced tissue with the corresponding volume of PBS (generally**

at a weight-to-volume ratio of 1:9, for example, 1g of tissue sample corresponds to 9mL of PBS. The specific volume can be adjusted appropriately according to experimental needs and recorded. It is recommended to add Protease inhibitor) was added to a glass homogenizer and ground thoroughly on ice. In order to further lyse tissue cells, the homogenate can be sonicated or frozen and thawed repeatedly. Finally, centrifuge the homogenate at  $5000 \times g$  for 5 to 10 minutes, and take the supernatant for detection.

**Urine - Collect in sterile tubes and centrifuge at  $2000 \times g$  for 20 minutes. Carefully collect the supernatant. If a precipitate forms, centrifuge again.**

**Nanjing BYabsience technology Co.,Ltd**

**Website: [www.byabsience.cn](http://www.byabsience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**

**Reagent preparation 1. Before use, all components must be rewarmed**

**for at least 60 minutes to ensure sufficient rewarming to room temperature.**

2. Concentrated washing liquid: The concentrated washing liquid taken out from the refrigerator will produce crystals. This is a normal phenomenon. Heating in a water bath will completely dissolve the crystals. Concentrated detergent and distilled water, dilute 1:20, that is, 1 part of concentrated detergent, add 19 parts of distilled water. 3. Substrate: Substrate solutions A and B, mix thoroughly at a volume of 1:1 before use, and use within 15 minutes after mixing.

**Operating procedures: Return all reagents and components to room temperature first. For standards, quality control materials and samples, it is recommended to make duplicate holes.**

- 1、按前面说明书描述的方法，配制好试剂盒各种组分的工作液。
- 2、从铝箔袋中取出所需板条，剩余的板条用自封袋密封放回冰箱。
- 3、设置标准品孔、0 值孔、空白孔和样本孔，标准品孔各加不同浓度的标准品 50 $\mu$ L，0 值孔加样本稀释液 50 $\mu$ L，空白孔不加，样本孔加待测样本 50 $\mu$ L。
- 4、除空白孔外，标准品孔、0 值孔和样本孔，加入辣根过氧化物酶（HRP）标记的检测抗体 100  $\mu$ L。
- 5、用封板膜盖住反应板，37 $^{\circ}$ C 水浴锅或恒温箱避光孵育 60min。
- 6、揭开封板膜，弃去液体，吸水纸上拍干，每孔加满洗涤液，静置 20S，甩去洗涤液，吸水纸上拍干，如此重复 5 次。若使用自动洗板机，请按洗板机操作程序进行洗板，添加浸泡 30s 的程序，可以提高检测的精度。洗板结束，加底物前，要在干净不掉屑的纸上，充分拍干反应板。（提示：为获得理想的实验结果，必须彻底移除残留液体。洗板完成之后，请立即进行下

步操作，不要让微孔板干燥。）7、将底物 A 和 B 按 1:1 体积充分混合，所有孔中加入底物混合液 100 $\mu$ L。用封板膜盖住反应板，37 $^{\circ}$ C 水浴锅或恒温箱避光孵育 15min。

8、所有孔加入终止液 50 $\mu$ L，在 450nm 波长酶标仪上读取各孔吸光度（OD 值）。

**Nanjing BYabscience technology Co.,Ltd**

网址：[www.byabscience.cn](http://www.byabscience.cn)

官方热线：025-5229-8998

监督电话：15950492658



**操作流程图**



1. 对应板孔中加入50μL标准品工作液或样本后，立即每孔加入100ulHRP酶标抗体工作液，37°C孵育60分钟



2. 弃掉板内液体，洗板5次



3. 每孔加入底物A溶液50ul，底物B溶液50ul



4. 每孔加入50μL终止液




5. 立即在450nm波长下读数，处理数据



## 结果计算

9、以标准品浓度做为横坐标，对应的吸光度（OD 值）作为纵坐标，利用计算机软件，采用四参数 Logistic 曲线拟合（4-pl），创建标准曲线方程，通过样品的吸光度（OD 值），利用方程计算样品的浓度值。【用 ELISA Calc 软件计算，标曲建议使用四参数拟合，但不是唯一拟合方式】10、如果样品被稀释，通过上述方法测得的浓度值，要乘以稀释倍数，才是样品的最终浓度。注意：实验者需根据自己的实验建立标准曲线。每次检测，每块酶标板都必须设立标准曲线。以下曲线仅供参考！

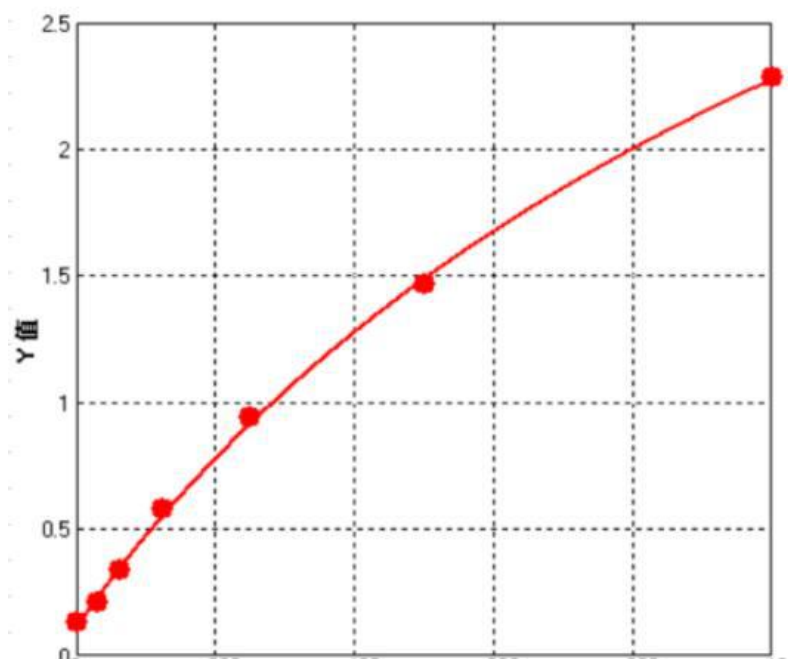

（标曲示意图，仅供参考）

Nanjing BYabscience technology Co.,Ltd



**[Problem Analysis]** If the experimental results are not good, please take pictures of the color development results in time, save the experimental data, keep the used strips and unused reagents, and then contact our company's technical support to solve the problem for you. At the same time, you can also refer to the following information:

**[Questions and Answers]**

Problem description	Possible reasons	Corresponding countermeasures
standard curve gradient difference	Incorrect liquid aspiration or	Check pipettes and tips
	Equilibration time is too short	Ensure sufficient balancing time
	Incomplete washing	Ensure the washing time and number of washings and the amount of liquid added to each hole
Very weak or colorless	Incubation time too short	Ensure adequate incubation time
	The experimental temperature is incorrect	Use recommended experimental temperatures
	Insufficient reagent volume or missing addition	Check the liquid aspirating and adding process to ensure that all reagents are added in order and in
	Incorrect dilution	
	Enzyme label inactivation or substrate failure	Mix enzyme conjugate and substrate and check by rapid color development
Reading value is low	Microplate reader settings are incorrect	Check the wavelength and filter
		Turn on the microplate reader and preheat it in advance
Large coefficient of variation	Adding fluid incorrectly	Check the filling situation
High background value	The working concentration of the	Use the recommended dilution
	Incomplete washing of enzyme plate	Ensure that each step of cleaning is complete; if using an automatic plate washer, please check whether all outlets are blocked;
	The lotion is contaminated	Prepare fresh lotion
Low sensitivity	Improper storage of ELISA kits	Store relevant reagents according to
	Not terminated before reading	Stop solution should be added to



# **Nanjing BYabscience technology Co.,Ltd**

**Website: [www.byabscience.cn](http://www.byabscience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**



## statement

1. Due to the current conditions and scientific and technological level, it is not possible to conduct comprehensive identification and analysis of all raw materials.  
This product may have certain quality and technical risks.
2. This kit removes/reduces some endogenous interfering factors in biological samples during the development process. Not all possible influencing factors have been removed.
3. The final experimental results are closely related to factors such as the effectiveness of the reagents, the relevant operations of the experimenter, and the experimental environment at the time. Our company is only responsible for the kit itself and is not responsible for the sample consumption caused by the use of the kit.  
Please use The user should fully consider the possible usage of the sample and reserve sufficient samples before use.
4. In order to achieve good experimental results, please only use the reagents provided in our company's kits, do not mix products from other manufacturers, and operate in strict accordance with the instructions.
5. Due to incorrect reagent preparation and microplate reader parameter settings during the operation, abnormal results may occur. Please read the instructions carefully and adjust the instrument before the experiment.
6. Even if operated by the same personnel, different results may be obtained in two independent experiments. In order to ensure the reproducibility of the results, it is necessary to control every step of the experimental process.

7. The kits will undergo strict quality inspection before shipment. However, due to factors such as transportation conditions, differences in experimental equipment, etc., user test results may be inconsistent with factory data.

8. This kit has not been compared with similar kits from other manufacturers or products using different methods to detect the same target, so inconsistent test results cannot be ruled out.

9. The kit is for research use only. If it is used for clinical diagnosis or any other purpose, our company will not be responsible for any problems arising therefrom, nor will we assume any legal liability.

**Nanjing BYabscience technology Co.,Ltd**

**Website: [www.byabscience.cn](http://www.byabscience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**