



**(For scientific research use only, not for clinical diagnosis!)**

## **Rabbit S100 Calbindin A8 (S100A8;MRP8) ELISA Kit**

**Instructions for Use Product No.: BY-ER772715**

**Specifications: 48T/96T Detection Range: 3.125 ng/mL–  
100 ng/mL.**

**Sensitivity: The lowest detectable dose is less than 0.1 ng/mL.**

**Precision: intra-batch variation coefficient CV% is less than 10%; inter-batch variation coefficient CV% is less than 15%.**

**Recovery rate: The recovery rate is between 85%-115%.**

**Specificity: This kit recognizes native and recombinant rabbit S100 calcium-binding protein A8 (S100A8; MRP8) and has no crossover with structural analogs.**

**Stability: Stored at 2°C-8°C, validity period is 6 months.**

**Purpose: Used to detect the concentration of rabbit S100 calcium-binding protein A8 (S100A8; MRP8) in samples such as serum, plasma, cell culture supernatant, and tissue.**

**Please read the instructions carefully before use. If you have any questions, please contact us through the following methods: Official hotline: 025-5229-**

**8998 Sales department phone: 13914481711 Technical phone: 15950492658**

**Company website: [www.byabscience.cn](http://www.byabscience.cn) For the specific shelf life, please**

**refer to the outer packaging label of the kit. Please use the kit within the**

**shelf life.**

**Nanjing BYabsience technology Co.,Ltd**

**Website: [www.byabsience.cn](http://www.byabsience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**




When contacting us, please provide the product number and production date (see box label) so that we can serve you more efficiently.



## Experimental principle

This kit uses a double-antibody sandwich enzyme-linked immunosorbent assay (ELISA). Add the rabbit S100 calcium-binding protein A8 (S100A8; Add HRP-labeled anti-rabbit S100 calcium-binding protein A8 (S100A8; MRP8) antibody (enzyme-labeled antibody), and after incubation and sufficient washing, unbound components are removed, and a solid-phase antibody-antigen is formed on the solid surface of the microplate. -Sandwich complex of enzyme-labeled antibodies. Adding substrates A and B, the substrates are catalyzed by HRP to produce a blue product, which is finally converted to yellow under the action of the stop solution (acidic solution). The absorbance (OD value) was measured on a microplate reader at a wavelength of 450 nm. The absorbance (OD value) was positively correlated with the concentration of rabbit S100 calcium-binding protein A8 (S100A8; MRP8) in the sample to be tested. By fitting the calibrator curve, the concentration of rabbit S100 calcium-binding protein A8 (S100A8; MRP8) in the sample can be calculated.

## Experimental schematic diagram

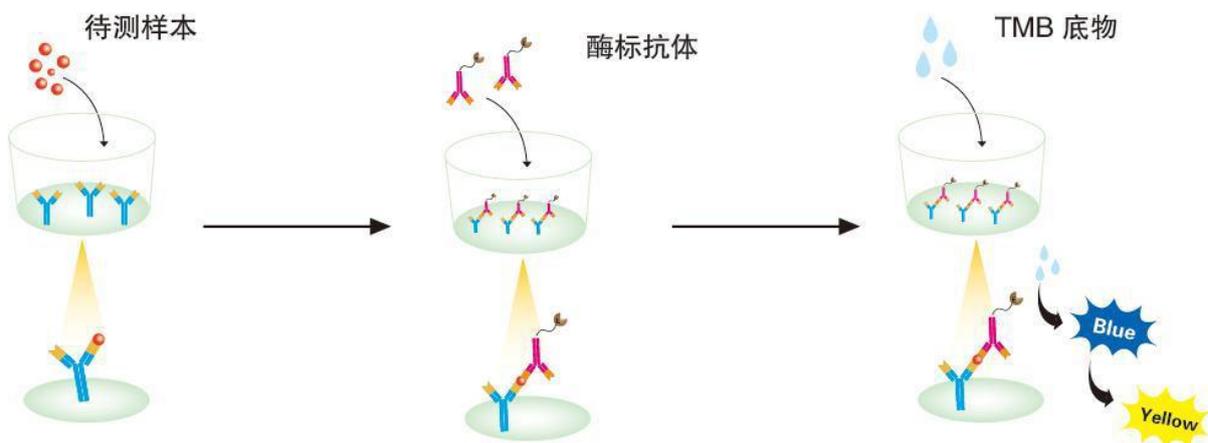

**Nanjing BYabscience technology Co.,Ltd**

**Website: [www.byabscience.cn](http://www.byabscience.cn)**

**Official hotline: 025-5229-8998**

**Supervision phone number:**



**Kit components and storage: Store unopened kits at 2-8 degrees Celsius. Do not use expired kits.**

Components	48-well configuration	96-well configuration	Store after opening
Pre-coated enzyme	48T	96T	<b>2-8°C 14 days</b>
Standard product	0.3mL*6 tubes	0.3mL*6 tubes	<b>2-8°C 14 days</b>
sample diluent	3ml	6ml	2-8°C 180 days
HRP labeled antibodies	5ml	10ml	<b>2-8°C 14 days</b>
Chromogenic substrate	3ml	6ml	2-8°C 180 days
Chromogenic substrate	3ml	6ml	2-8°C 180 days
stop solution	3ml	6ml	2-8°C 180 days
<b>20×Lotion</b>	15ml	25ml	2-8°C 180 days
sealing film	2 sheets	2 sheets	
manual	1 serving	1 serving	
Ziplock bag	1	1	

The concentrations of calibrators are: 100, 50, 25, 12.5, 6.25, 3.125 ng/mL.

Note: 1: Before use, please check whether the label and quantity of

the reagents in the kit are consistent with the table.

2: If the components of the kit need to be used again, please ensure that they have

not been contaminated since the last use. 3: If the enzyme plate is not used up in a

single time, remember to seal it and store it at 2-8°C.

**试验所需自备试验器材 (不提供, 但可协助购买)**

1) 能够检测 450 nm 吸光度的酶标仪 2)

移液器及枪头、加样槽 3) 37°C 恒温箱或

水浴锅 4) 准备试剂用的试管、离心管、

量筒等 5) 蒸馏水或去离子水

**Nanjing BYabscience technology Co.,Ltd**

网址: [www.byabscience.cn](http://www.byabscience.cn)

官方热线: 025-5229-8998

监督电话: 15950492658



## 6) 涡旋振荡器、微孔板振荡器

**注意事项 1) 仅供科研使用，不得用于临床诊断。**

- 2) 在试剂盒标示的有效期内使用，过期产品不得使用。
- 3) 跟其他厂家的试剂盒或者组分不能混用，使用试剂盒配套的样品稀释液。
- 4) 如果样本值高于最高标准品浓度值，请将样本适当稀释后，再重新测定。
- 5) 待测样本中存在的人抗鼠等异嗜抗体会干扰检测结果，检测前，请排出该因素。
- 6) 通过其他方法得到的检测结果，与本试剂盒测定结果不具有直接的可比性。
- 7) 试验中请穿着实验服并戴乳胶手套做好防护工作。特别是检测血液或者其他体液样品时，请按国家生物试验室安全防护条例执行。
- 8) 严格按照规定的时间和温度进行温育以保证准确结果。所有试剂都必须在使用前达到室温 20-25°C。使用后立即冷藏保存试剂。
- 9) 洗板不正确可以导致不准确的结果。在加入底物前确保尽量吸干孔内液体。温育过程中不要让微孔干燥掉。
- 10) 消除板底残留的液体和手指印，否则影响 OD 值。
- 11) 底物显色液应呈无色或很浅的颜色。
- 12) 避免试剂和标本的交叉污染以免造成错误结果。
- 13) 在储存和温育时避免强光直接照射。
- 14) 检测使用的酶标仪需要安装能检测 450±10nm 波长的滤光片，光密度范围在 0-3.5 之间。建议使用时提前 15 分钟预热。
- 15) 试验中所用的 EP 管和吸头均为一次性使用，严禁混用。





## 样品的准备和保存

以下只是列出样品采集和保存的一般指南。所有样本采集保存过程中，不得使用叠氮钠做为防腐剂。样品如果不立即分析，应分装后冷冻保存，且避免反复冻融。

**细胞培养上清**——离心去除沉淀，立即分析或分装后-20℃冷冻保存。

**血清**——用干净试管收集血液，室温凝固 30 分钟，离心 2000×g 20 分钟，收集血清。立即分析或分装后-20℃冷冻保存。

**血浆**——采用肝素、柠檬酸盐或 EDTA 抗凝，抽血后 30 分钟内在 2-8℃离心 2000×g 20 分钟。为消除血小板的影响，建议在 2-8℃进一步离心 10000×g 10 分钟。立即分析或分装后-20℃冷冻保存。

**细胞裂解液**——对于贴壁细胞，去除培养液，用 PBS、生理盐水或无血清培养液洗一遍。加入适量裂解液，用枪吹打数下，使裂解液和细胞充分接触。通常 10 秒后，细胞就会被裂解。对于悬浮细胞，离心收集细胞，用 PBS、生理盐水或无血清培养液洗一遍。加入适量裂解液，用枪吹打把细胞吹散，用手指轻弹以充分裂解细胞。充分裂解后，10000—14000×g 离心 3-5 分钟，取上清。立即分析或分装后-20℃冷冻保存。

**组织匀浆**——用预冷的 PBS (0.01M, pH=7.4)冲洗组织，去除残留血液（匀浆中裂解的红细胞会影响测量结果），称重后将组织剪碎。将剪碎的组织与对应体积的 PBS（一般按 1:9 的重量体积比，比如 1g 的组织样品对应 9mL 的 PBS，具体体积可根据实验需要适当调整，并做好记录。推荐在 PBS 中加入蛋白酶抑制剂）加入玻璃匀浆器中，于冰上充分研磨。为了进一步裂解组织细胞，可以对匀浆液进行超声破碎，或反复冻融。最后将匀浆液于 5000×g 离心 5~10 分钟，取上清检测。

**尿液**——用无菌管收集，离心 2000×g 20 分钟。仔细收集上清。如有沉淀形成，应再次离心。



试剂准备 1、使用前，所有的组分都要至少复温 60min，确保充分复温到室温。

2、浓缩洗涤液：从冰箱取出的浓缩洗涤液，会有结晶产生，这属于正常现象，水浴加热使结晶完全溶解。浓缩洗涤液与蒸馏水，按 1:20 稀释，即 1 份的浓缩洗涤液，添加 19 份的蒸馏水。3、底物：底物液 A 和 B，在使用前，按 1:1 体积充分混合，混合后 15 分钟内使用。


操作程序 所有试剂和组分都先恢复到室温，标准品、质控品和样品，建议做复孔。

- 1、按前面说明书描述的方法，配制好试剂盒各种组分的工作液。
- 2、从铝箔袋中取出所需板条，剩余的板条用自封袋密封放回冰箱。
- 3、设置标准品孔、0 值孔、空白孔和样本孔，标准品孔各加不同浓度的标准品 50 $\mu$ L，0 值孔加样本稀释液 50 $\mu$ L，空白孔不加，样本孔加待测样本 50 $\mu$ L。
- 4、除空白孔外，标准品孔、0 值孔和样本孔，加入辣根过氧化物酶（HRP）标记的检测抗体 100  $\mu$ L。
- 5、用封板膜盖住反应板，37 $^{\circ}$ C 水浴锅或恒温箱避光孵育 60min。
- 6、揭开封板膜，弃去液体，吸水纸上拍干，每孔加满洗涤液，静置 20S，甩去洗涤液，吸水纸上拍干，如此重复 5 次。若使用自动洗板机，请按洗板机操作程序进行洗板，添加浸泡 30s 的程序，可以提高检测的精度。洗板结束，加底物前，要在干净不掉屑的纸上，充分拍干反应板。（提示：为获得理想的实验结果，必须彻底移除残留液体。洗板完成之后，请立即进行下一步操作，不要让微孔板干燥。）
- 7、将底物 A 和 B 按 1:1 体积充分混合，所有孔中加入底物混合液 100 $\mu$ L。用封板膜盖住反应板，37 $^{\circ}$ C 水浴锅或恒温箱避光孵育 15min。
- 8、所有孔加入终止液 50 $\mu$ L，在 450nm 波长酶标仪上读取各孔吸光度（OD 值）。






操作流程图

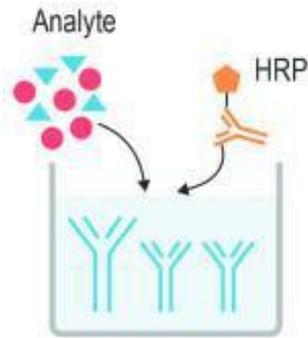


1. 对应板孔中加入50 $\mu$ L标准品工作液或样本后，立即每孔加入100ulHRP酶标抗体工作液，37 $^{\circ}$ C孵育60分钟



2. 弃掉板内液体，洗板5次



3. 每孔加入底物A溶液50ul，底物B溶液50ul



4. 每孔加入50 $\mu$ L终止液




5. 立即在450nm波长下读数，处理数据



## 结果计算

9、以标准品浓度做为横坐标，对应的吸光度（OD 值）作为纵坐标，利用计算机软件，采用四参数 Logistic 曲线拟合（4-p1），创建标准曲线方程，通过样品的吸光度（OD 值），利用方程计算样品的浓度值。【用 ELISA Calc 软件计算，标曲建议使用四参数拟合，但不是唯一拟合方式】10、如果样品被稀释，通过上述方法测的的浓度值，要乘以稀释倍数，才是样品的最终浓度。注意：实验者需根据自己的实验建立标准曲线。每次检测，每块酶标板都必须设立标准曲线。以下曲线仅供参考！

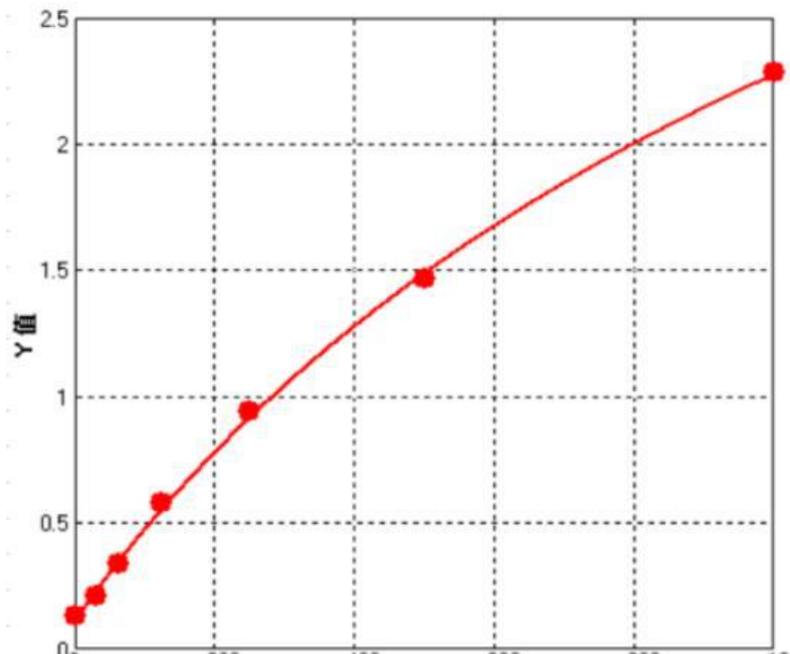

（标曲示意图，仅供参考）



**[Problem Analysis] If the experimental results are not good, please take pictures of the color development results in time, save the experimental data, keep the used strips and unused reagents, and then contact our company's technical support to solve the problem for you. At the same time, you can also refer to the following information:**

**[Questions and Answers]**

Problem description	Possible reasons	Corresponding countermeasures Corresponding countermeasures
standard curve gradient difference	Incorrect liquid aspiration or	Check pipettes and tips
	Equilibration time is too short	Ensure sufficient balancing time
	Incomplete washing	Ensure the washing time and number of washes and the amount of liquid added to each hole
Very weak or colorless	Incubation time too short	Ensure adequate incubation time
	The experimental temperature is incorrect	Use recommended experimental temperatures
	Insufficient reagent volume or missing addition	Check the liquid aspiration and addition process to ensure that all reagents are added in sufficient
	Incorrect dilution	
Enzyme label inactivation or substrate failure	Mix enzyme conjugate and substrate and check by rapid color development	
Reading value is low	Microplate reader settings are incorrect	Check the wavelength and filter
		Turn on the microplate reader and preheat it in advance
Large coefficient of variation	Adding fluid incorrectly	Check the filling situation
High background value	The working concentration of the	Use the recommended dilution
	Incomplete washing of enzyme plate	Ensure that each step of cleaning is complete; if using an automatic plate washer, please check whether all outlets are blocked;
	The lotion is contaminated	Prepare fresh lotion
Low sensitivity	Improper storage of ELISA kits	Store relevant reagents according to
	Not terminated before reading	Stop solution should be added to

# Nanjing BYabscience technology Co.,Ltd

Website: [www.byabscience.cn](http://www.byabscience.cn)

Official hotline: 025-5229-8998

Supervision phone number:



## statement

1. Due to the current conditions and scientific and technological level, it is not possible to conduct comprehensive identification and analysis of all raw materials. This product may have certain quality and technical risks.
2. This kit removes/reduces some endogenous interfering factors in biological samples during the development process. Not all possible influencing factors have been removed.
3. The final experimental results are closely related to factors such as the effectiveness of the reagents, the relevant operations of the experimenter, and the experimental environment at the time. Our company is only responsible for the kit itself and is not responsible for the sample consumption caused by the use of the kit. Please use The user should fully consider the possible usage of the sample and reserve sufficient samples before use.
4. In order to achieve good experimental results, please only use the reagents provided in our company's kits, do not mix products from other manufacturers, and operate in strict accordance with the instructions.
5. 由于操作过程中试剂制备以及酶标仪参数设置不正确，可能导致结果异常，实验前请仔细阅读说明书并调整好仪器。
6. 即使是相同人员操作也可能在两次独立实验中得到不同的结果，为保证结果的重现性，需要控制实验过程中每一步的操作。
7. 试剂盒发货前会经过严格的质检，然而，因为运输条件、实验设备差异等等因素影响，用户检测结果可能跟出厂数据不一致。

8. 本试剂盒未与其他厂家同类试剂盒或不同方法检测同一目的物的产品进行对比，所以不排除检测结果不一致的情况。

9. 试剂盒仅供研究使用，如将其用于临床诊断或任何其他用途，我公司将不对因此产生的问题负责，亦不承担任何法律责任。

**Nanjing BYabscience technology Co.,Ltd**

网址：[www.byabscience.cn](http://www.byabscience.cn)

官方热线：025-5229-8998

监督电话：15950492658